



1 Preparation

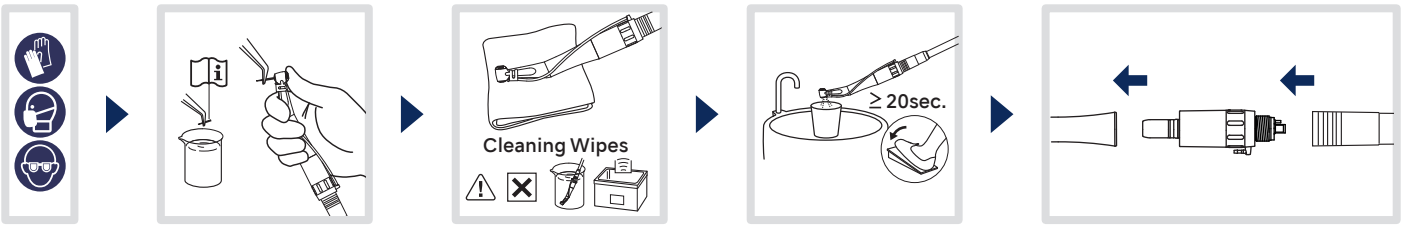


2 Cleaning and Drying

Manual

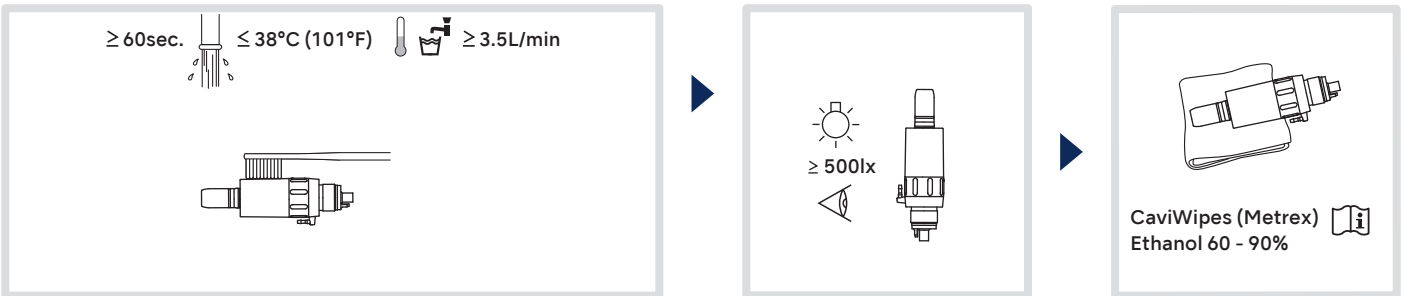

- ⚠ After cleaning, if moisture is present, wipe off with a dry cloth or blow it off with compressed air until there is no moisture in the interior and exterior.
- When blowing off with compressed air, cover the product with cloth to prevent scattering of water.
- Use a state-sanctioned disinfectant with proven bactericidal, fungicidal, and virucidal properties.

3 Cleaning and Lubrication

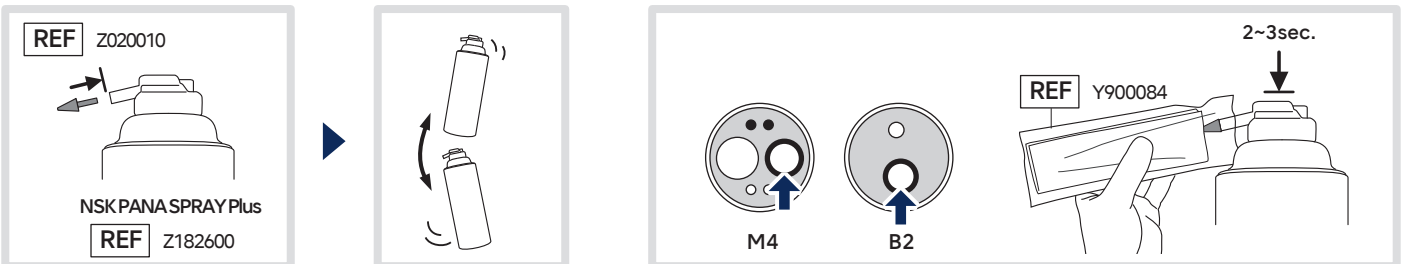

4 Packaging, Sterilizing, and Drying

ISO 11607-1

Use an FDA-approved sterilization pouch that conforms to ISO 11607-1, and seal the pouch. Maximum temperature for NSK instruments is 135°C (275°F).

Type	Gravity Displacement	Pre-Vacuum (Dynamic Air Removal)
Temperature	132°C (270°F)	132°C (270°F)
Full Cycle Time	15min	4min
Drying Time	30min	30min


Perform steam sterilization with the above conditions. Use an FDA-approved steam sterilizer to perform sterilization.

CAUTION

Steam sterilization

Plasma EO

5 Storage



NSK America Corp.

1800 Global Parkway, Hoffman Estates, IL 60192, USA
 TEL: +1 888 675 1675 FAX: +1 800 838 9328