


### 1 Preparation

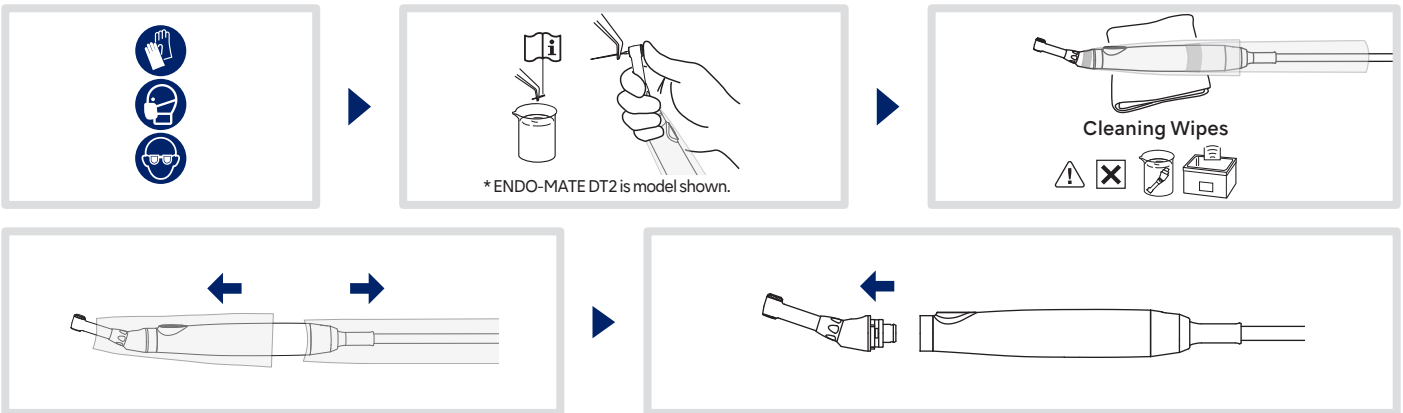


⚠ · Use a disposable barrier sleeve that meets local regulations.


### 2 Cleaning and Drying

#### ■ Contra Angle head

##### Manual

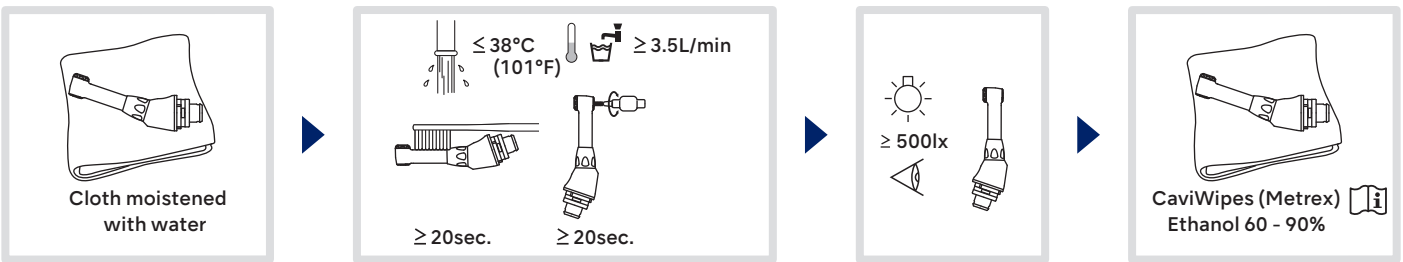


##### Automated

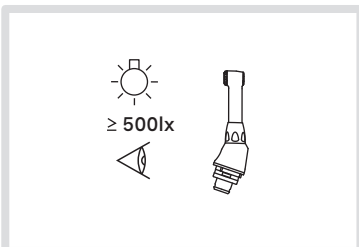


⚠ · After cleaning, if moisture is present, wipe off with a dry cloth or blow it off with compressed air until there is no moisture in the interior and exterior.  
 · When blowing off with compressed air, cover the product with cloth to prevent scattering of water.  
 · Use a state-sanctioned disinfectant with proven bactericidal, fungicidal, and virucidal properties.


#### ■ Control unit

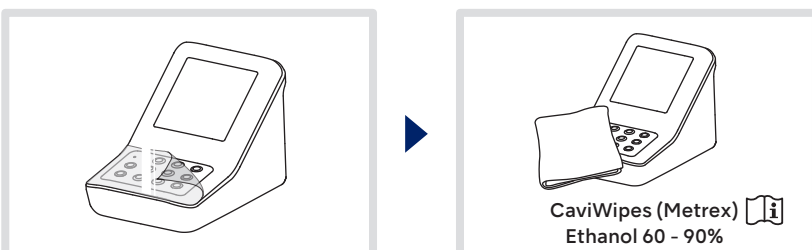


## Motor handpiece

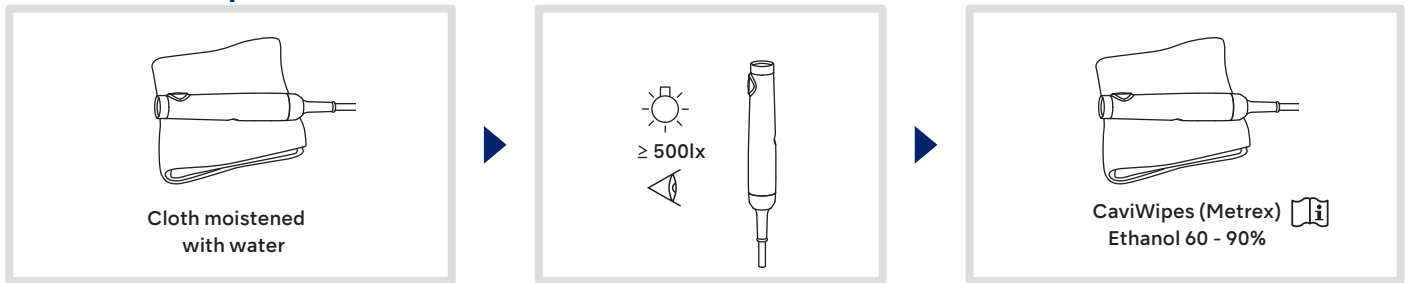

## Handpiece stand

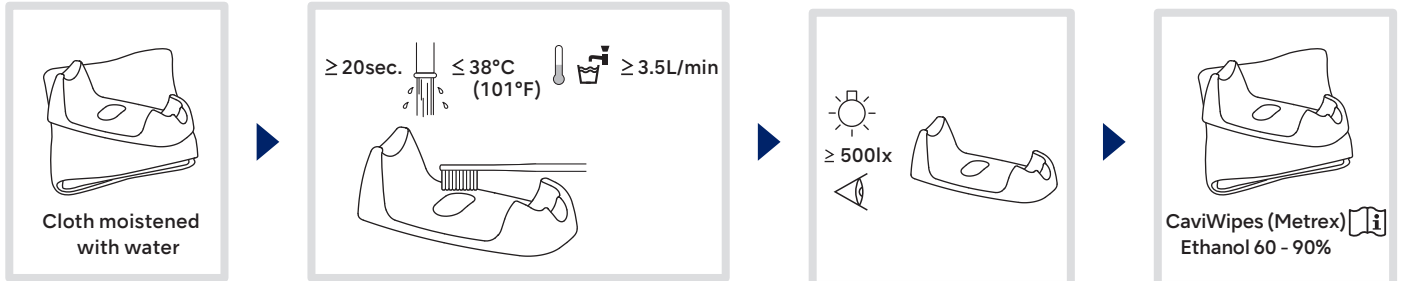

## 3 Cleaning and Lubrication

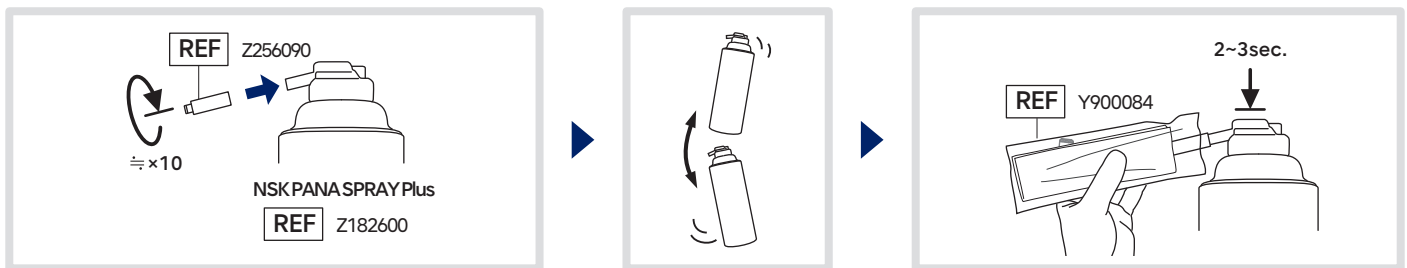

## 4 Packaging, Sterilizing, and Drying

ISO 11607-1

135°C

Type	Gravity Displacement	Pre-Vacuum (Dynamic Air Removal)
Temperature	132°C (270°F)	132°C (270°F)
Full Cycle Time	15min	4min
Drying Time	30min	30min

CAUTION

Steam sterilization

Plasma

EO

Use an FDA-approved sterilization pouch that conforms to ISO 11607-1, and seal the pouch. Maximum temperature for NSK instruments is 135°C (275°F).

Perform steam sterilization with the above conditions. Use an FDA-approved steam sterilizer to perform sterilization.

## 5 Storage

